


JAN 18 2011
2011
3/9/11

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

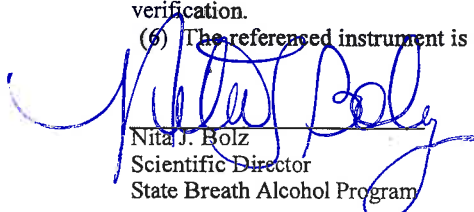
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130187 ✓		
Supervisor/Operator Performing the Verification Procedure:		
Name	Dan Pasquariello	ID# 2620 ✓ Date 1-11-11 ✓
A	Agency Dillingham PD	Phone # 842-5354
Instrument Location Dillingham PD		
Alco S/N 70108 ✓ Target Value .081 ✓ High Pressure 850 psi		
B	Alco Test Values	
	1st Alco .085 ✓	2nd Alco .085 ✓
Signature 		
(OVER)		


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 11th day of MAR, 2011.


Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office

(Notary Seal Stamp)



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130187

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130187

JANUARY 11, 2011

OPERATOR'S NAME:

PASQUARIELLO, DAN

OPERATOR'S NUMBER: 2620

SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/MI :

VOC

O.L. #: 1234567890

DEPT/AGENCY: DL61

CASE/REPORT: 1234567890

TEST TYPE: U

ALCO TARGET VALUE: .081

ALCO S/N: 70100

— BREATH ANALYSIS —

.081 ADJUSTED FOR 30.64 in
ALCO TARGET .082 19:12
BLANK TEST .000 19:13
INTERNAL STANDARD VERIFIED 19:13
ALCO TO 30.64 in .085 19:14
BLANK TEST .000 19:15
SUBJECT SAMPLE .000 19:15
BLANK TEST .000 19:16
ALCO TO 30.64 in .085 19:16
BLANK TEST .000 19:17

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130187

JANUARY 11, 2011

TIME 19:18

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 30.64 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~ ¡ ¢